


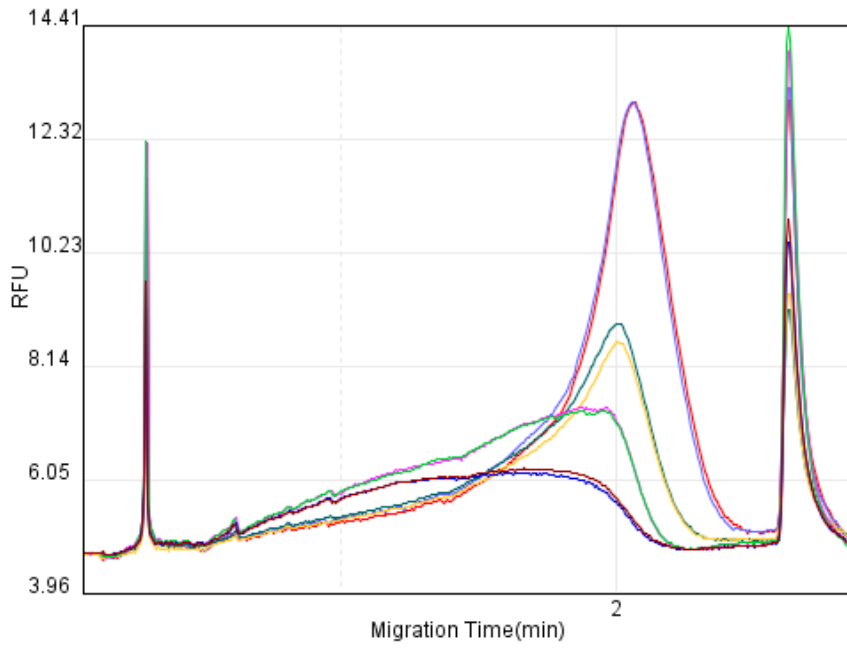
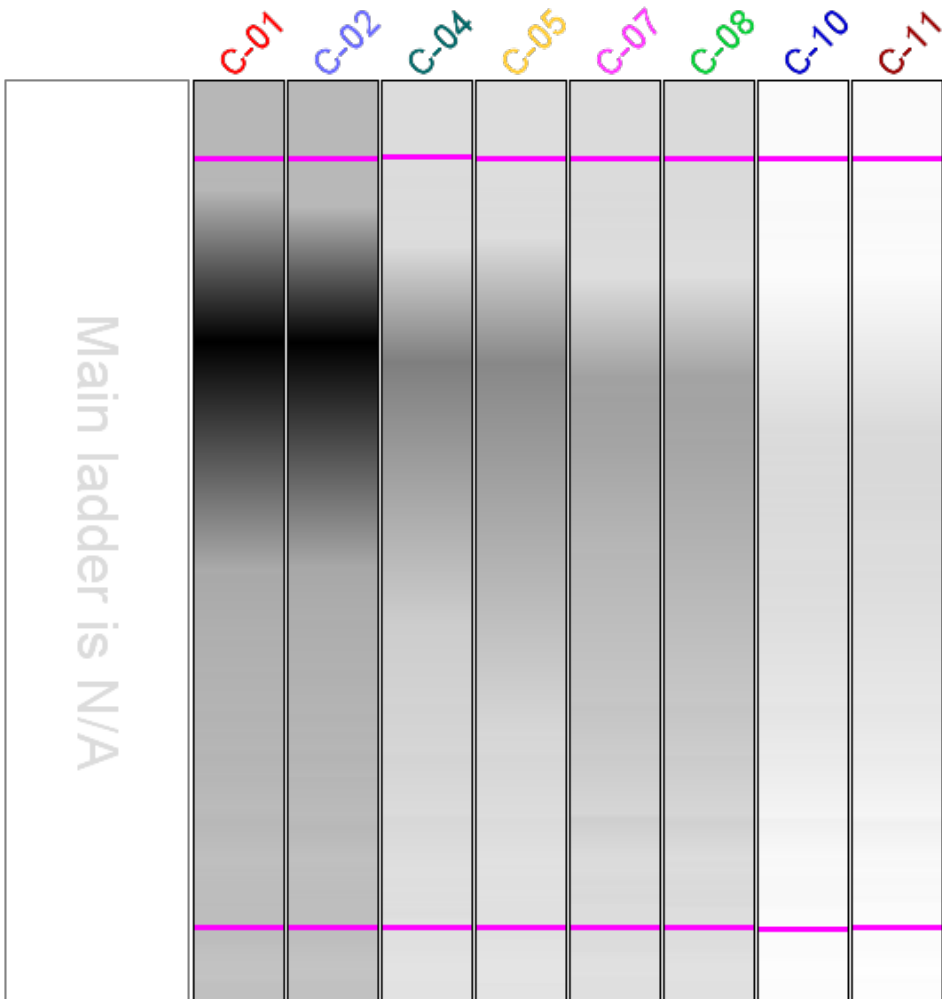
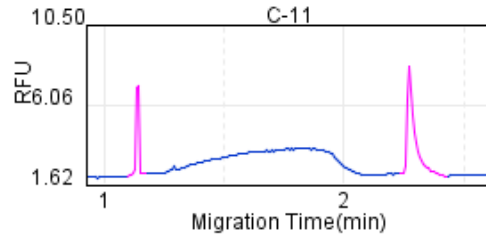
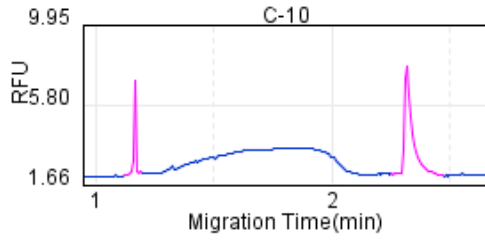
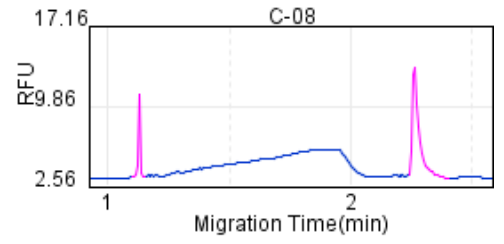
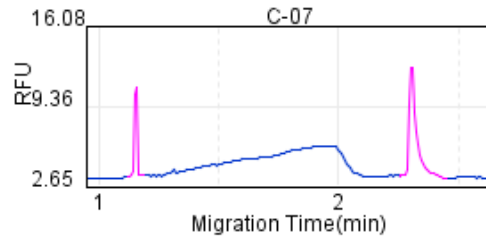
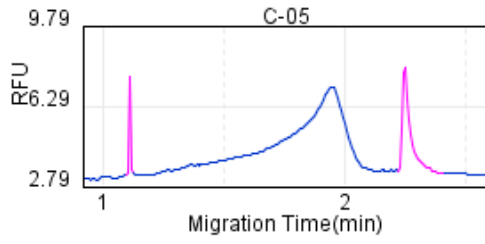


File Summary

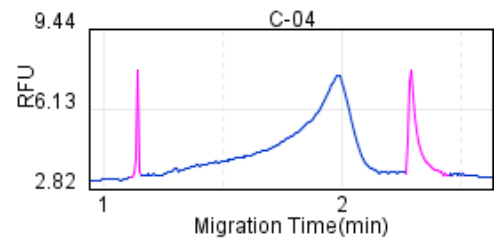

File Name	
1	20260319_S1C01_R1_CH1.bopx
2	20260319_S1C02_R1_CH1.bopx
3	20260319_S1C04_R1_CH2.bopx
4	20260319_S1C05_R1_CH2.bopx
5	20260319_S1C07_R1_CH3.bopx
6	20260319_S1C08_R1_CH3.bopx
7	20260319_S1C10_R1_CH4.bopx
8	20260319_S1C11_R1_CH4.bopx

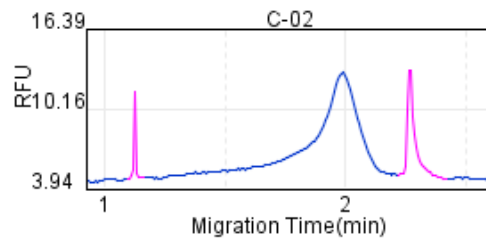

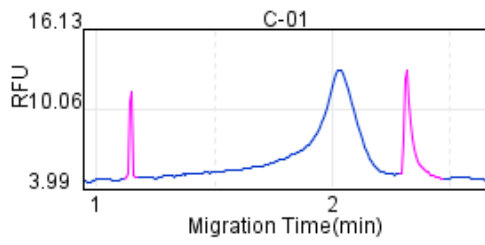

Result: 1-20260319\_S1C01\_R1\_CH1.bopx

Test Time: 2026-Mar-21 14:32(UTC+08)

Instrument ID:

5567003745270004

Operator:

Software & Firmware Version:

3.4.3 & 5

Method: M-4-10-08-160

Cartridge & Run Number:

S2-O-4CH-250918-115 & 23

Sample Name:


Manufacture & Expiration Date:

2025-Sep-18 & 2026-Mar-17

Sample ID: 1-20260319

Alignment Marker:

UserDefine (20 bp & 5K bp)

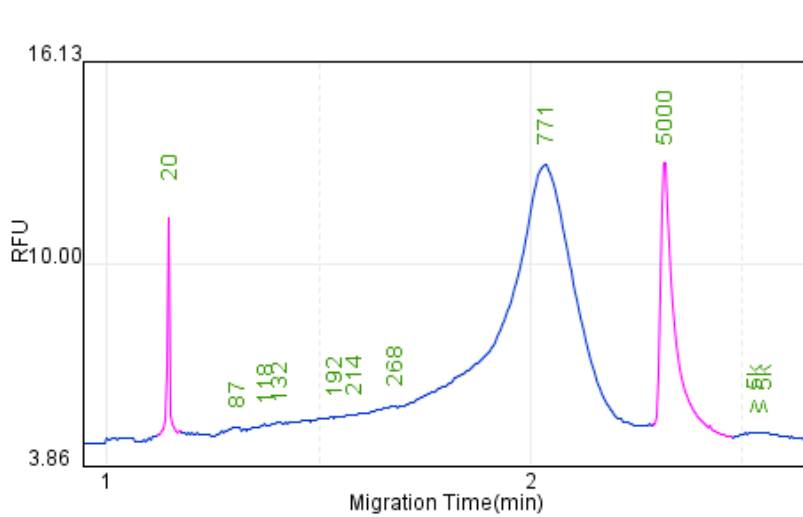

No	bp	ng/μl
1	<LM	N/A
2	20	N/A
3	87	0.08
4	118	0.10
5	132	0.11
6	147	0.08
7	161	0.07
8	192	0.21
9	214	0.20
10	268	0.57
11	771	8.56
12	3,667	<0.01
13	3,954	0.02
14	5,000	N/A
15	> 5k	N/A
16	> 5k	N/A
17	> 5k	N/A
18	> 5k	N/A
19	> 5k	N/A
20	> 5k	N/A

Result: 2-20260319\_S1C02\_R1\_CH1.bopx

Test Time: 2026-Mar-21 14:38(UTC+08)

Instrument ID:

5567003745270004

Operator:

Software & Firmware Version:

3.4.3 & 5

Method: M-4-10-08-160

Cartridge & Run Number:

S2-O-4CH-250918-115 & 22

Sample Name:


Manufacture & Expiration Date:

2025-Sep-18 & 2026-Mar-17

Sample ID: 2-20260319

Alignment Marker:


UserDefine (20 bp & 5K bp)

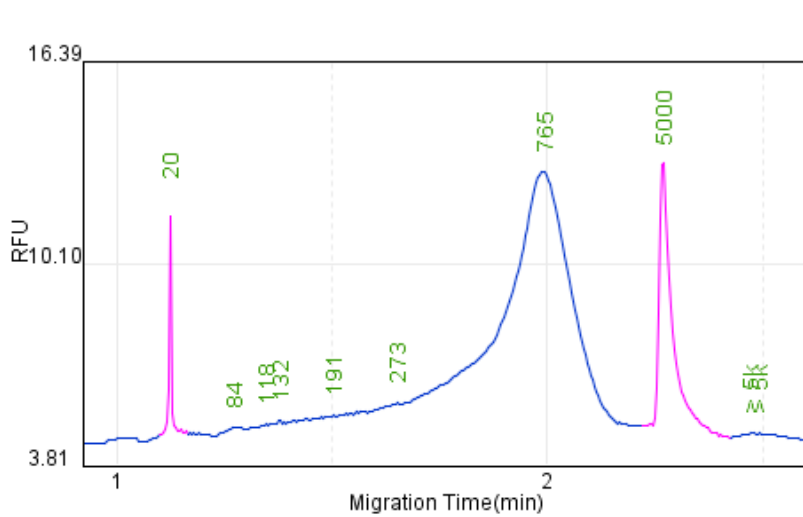

No	bp	ng/μl
1	<LM	N/A
2	20	N/A
3	37	<0.01
4	84	0.08
5	118	0.13
6	132	0.13
7	146	0.10
8	161	0.05
9	191	0.25
10	213	0.18
11	229	0.15
12	273	0.48
13	765	8.57
14	3,206	0.03
15	3,527	0.02
16	5,000	N/A
17	> 5k	N/A
18	> 5k	N/A
19	> 5k	N/A
20	> 5k	N/A
21	> 5k	N/A
22	> 5k	N/A
23	> 5k	N/A
24	> 5k	N/A

---

Result:	3-20260319_S1C04_R1_CH2.bopx	Instrument ID:	5567003745270004
Test Time:	2026-Mar-21 14:32(UTC+08)	Software & Firmware Version:	3.4.3 & 5
Operator:		Cartridge & Run Number:	S2-O-4CH-250918-115 & 23
Method:	M-4-10-08-160	Manufacture & Expiration Date:	2025-Sep-18 & 2026-Mar-17
Sample Name:		Alignment Marker:	UserDefine (20 bp & 5K bp)
Sample ID:	3-20260319		

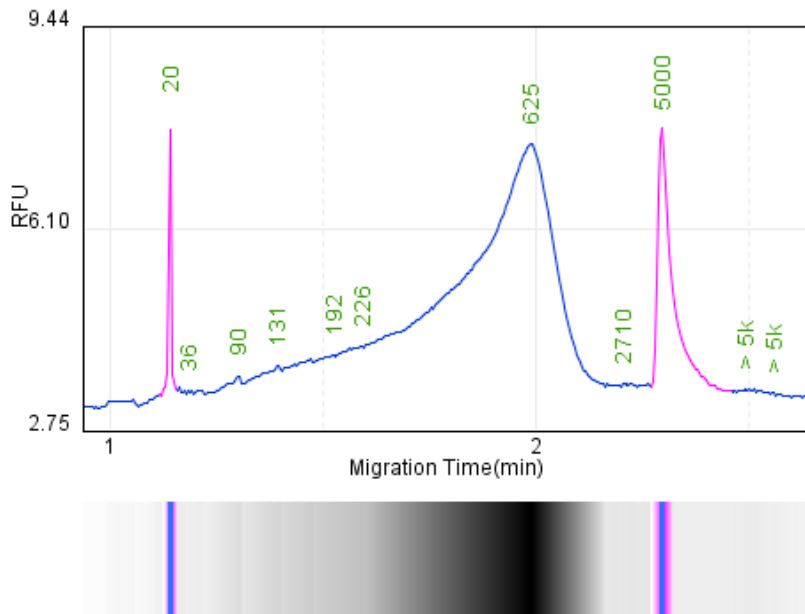

No	bp	ng/μl
1	<LM	N/A
2	<LM	N/A
3	<LM	N/A
4	<LM	N/A
5	20	N/A
6	36	<0.01
7	90	0.09
8	131	0.22
9	148	0.10
10	168	0.10
11	192	0.19
12	226	0.28
13	625	5.52
14	2,106	0.01
15	2,305	0.03
16	2,710	0.01
17	3,047	0.03
18	3,939	0.03
19	5,000	N/A
20	> 5k	N/A
21	> 5k	N/A
22	> 5k	N/A
23	> 5k	N/A
24	> 5k	N/A
25	> 5k	N/A
26	> 5k	N/A
27	> 5k	N/A
28	> 5k	N/A
29	> 5k	N/A
30	> 5k	N/A
31	> 5k	N/A
32	> 5k	N/A
33	> 5k	N/A
34	> 5k	N/A
35	> 5k	N/A
36	> 5k	N/A
37	> 5k	N/A
38	> 5k	N/A
39	> 5k	N/A
40	> 5k	N/A
41	> 5k	N/A
42	> 5k	N/A
43	> 5k	N/A

Result: 4-20260319\_S1C05\_R1\_CH2.bopx

Test Time: 2026-Mar-21 14:38(UTC+08)

Instrument ID:

5567003745270004

Operator:

Software & Firmware Version:

3.4.3 & 5

Method: M-4-10-08-160

Cartridge & Run Number:

S2-O-4CH-250918-115 & 22

Sample Name:


Manufacture & Expiration Date:

2025-Sep-18 & 2026-Mar-17

Sample ID: 4-20260319

Alignment Marker:

UserDefine (20 bp & 5K bp)

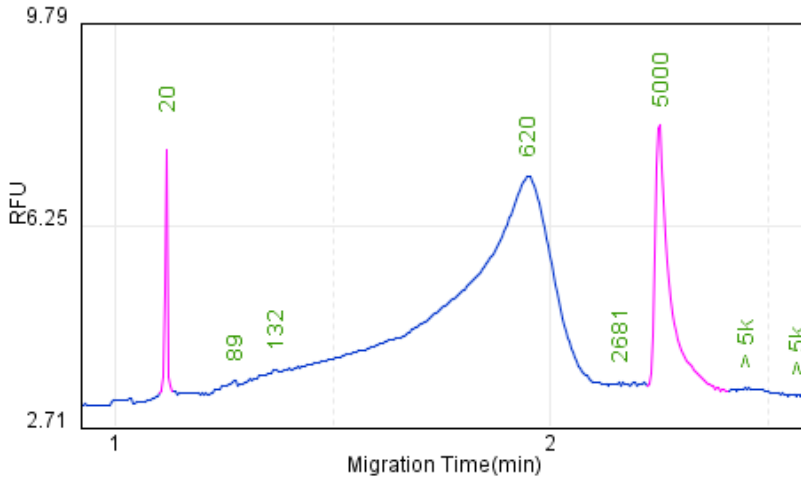

No	bp	ng/μl
1	<LM	N/A
2	<LM	N/A
3	<LM	N/A
4	20	N/A
5	89	0.06
6	132	0.21
7	145	0.08
8	620	5.62
9	2,681	0.03
10	2,925	0.02
11	3,356	0.02
12	3,886	0.01
13	5,000	N/A
14	> 5k	N/A
15	> 5k	N/A
16	> 5k	N/A
17	> 5k	N/A
18	> 5k	N/A
19	> 5k	N/A
20	> 5k	N/A
21	> 5k	N/A
22	> 5k	N/A
23	> 5k	N/A
24	> 5k	N/A
25	> 5k	N/A
26	> 5k	N/A
27	> 5k	N/A
28	> 5k	N/A
29	> 5k	N/A
30	> 5k	N/A
31	> 5k	N/A
32	> 5k	N/A

Result: 5-20260319\_S1C07\_R1\_CH3.bopx

Test Time: 2026-Mar-21 14:32(UTC+08)

Instrument ID:

5567003745270004

Operator:

Software & Firmware Version:

3.4.3 & 5

Method: M-4-10-08-160

Cartridge & Run Number:

S2-O-4CH-250918-115 & 23

Sample Name:


Manufacture & Expiration Date:

2025-Sep-18 & 2026-Mar-17

Sample ID: 5-20260319


Alignment Marker:

UserDefine (20 bp & 5K bp)

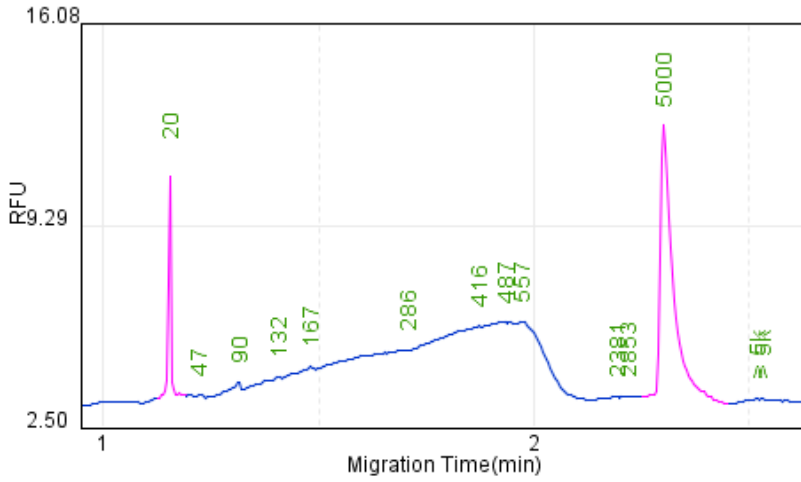

No	bp	ng/μl
1	<LM	N/A
2	<LM	N/A
3	20	N/A
4	37	0.03
5	47	0.03
6	59	0.02
7	90	0.18
8	132	0.41
9	167	0.31
10	286	2.04
11	416	1.94
12	487	0.82
13	497	0.20
14	557	1.14
15	1,542	<0.01
16	2,381	0.03
17	2,853	0.02
18	3,482	0.02
19	5,000	N/A
20	> 5k	N/A
21	> 5k	N/A
22	> 5k	N/A
23	> 5k	N/A
24	> 5k	N/A
25	> 5k	N/A
26	> 5k	N/A
27	> 5k	N/A
28	> 5k	N/A
29	> 5k	N/A
30	> 5k	N/A
31	> 5k	N/A
32	> 5k	N/A
33	> 5k	N/A
34	> 5k	N/A
35	> 5k	N/A

Result: 6-20260319\_S1C08\_R1\_CH3.bopx  
 Test Time: 2026-Mar-21 14:38(UTC+08) Instrument ID: 5567003745270004  
 Operator: Software & Firmware Version: 3.4.3 & 5  
 Method: M-4-10-08-160 Cartridge & Run Number: S2-O-4CH-250918-115 & 22  
 Sample Name: Manufacture & Expiration Date: 2025-Sep-18 & 2026-Mar-17  
 Sample ID: 6-20260319 Alignment Marker: UserDefine (20 bp & 5K bp)

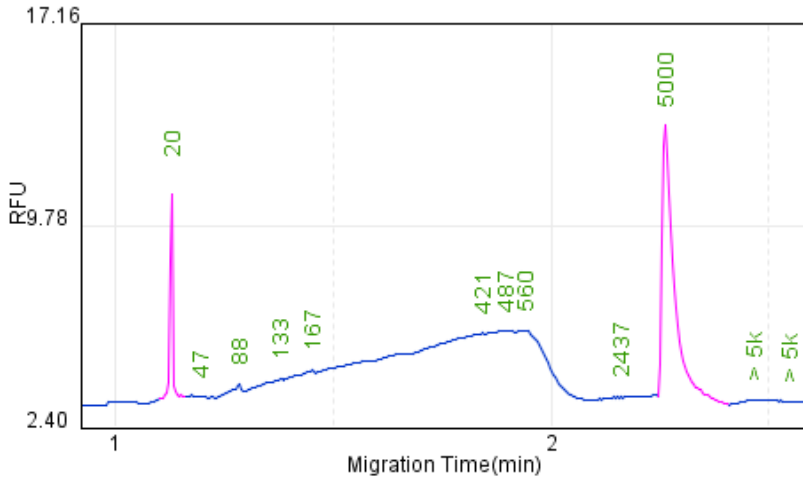

No	bp	ng/μl
1	<LM	N/A
2	20	N/A
3	33	0.01
4	37	0.03
5	47	0.03
6	59	0.02
7	88	0.18
8	133	0.39
9	167	0.31
10	421	3.82
11	487	0.93
12	560	1.08
13	1,514	<0.01
14	2,437	0.04
15	2,874	0.03
16	3,327	<0.01
17	3,451	0.02
18	4,145	0.02
19	5,000	N/A
20	> 5k	N/A
21	> 5k	N/A
22	> 5k	N/A
23	> 5k	N/A
24	> 5k	N/A
25	> 5k	N/A
26	> 5k	N/A
27	> 5k	N/A
28	> 5k	N/A
29	> 5k	N/A
30	> 5k	N/A
31	> 5k	N/A
32	> 5k	N/A
33	> 5k	N/A
34	> 5k	N/A
35	> 5k	N/A

Result: 7-20260319\_S1C10\_R1\_CH4.bopx

Test Time: 2026-Mar-21 14:32(UTC+08)

Instrument ID:

5567003745270004

Operator:

Software & Firmware Version:

3.4.3 & 5

Method: M-4-10-08-160

Cartridge & Run Number:

S2-O-4CH-250918-115 & 23

Sample Name:


Manufacture & Expiration Date:

2025-Sep-18 & 2026-Mar-17

Sample ID: 7-20260319

Alignment Marker:

UserDefine (20 bp & 5K bp)

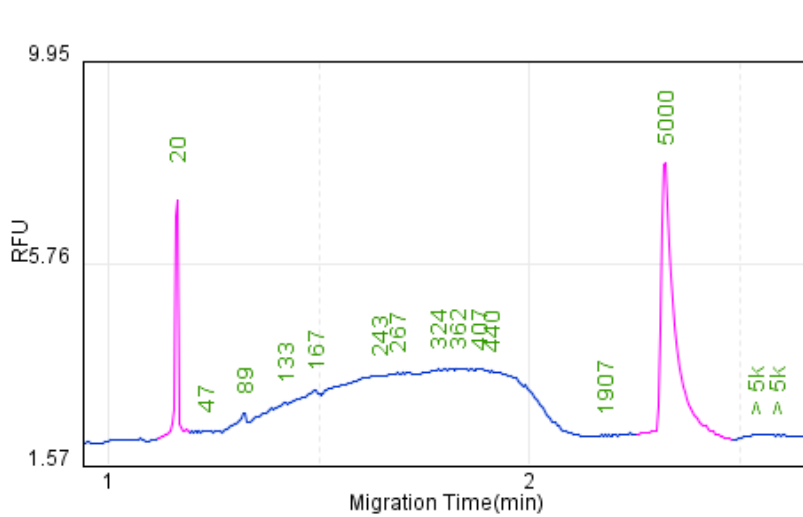

No	bp	ng/μl
1	<LM	N/A
2	20	N/A
3	33	0.01
4	37	0.01
5	47	0.04
6	61	0.03
7	89	0.15
8	133	0.37
9	167	0.27
10	243	1.18
11	267	0.43
12	278	0.22
13	315	0.46
14	324	0.09
15	336	0.12
16	352	0.16
17	362	0.27
18	391	0.09
19	407	0.28
20	440	0.89
21	1,907	<0.01
22	2,312	<0.01
23	2,999	0.01
24	5,000	N/A
25	> 5k	N/A
26	> 5k	N/A
27	> 5k	N/A
28	> 5k	N/A
29	> 5k	N/A
30	> 5k	N/A
31	> 5k	N/A
32	> 5k	N/A
33	> 5k	N/A
34	> 5k	N/A

Result: 8-20260319\_S1C11\_R1\_CH4.bopx

Test Time: 2026-Mar-21 14:38(UTC+08)

Instrument ID:

5567003745270004

Operator:

Software & Firmware Version:

3.4.3 & 5

Method: M-4-10-08-160

Cartridge & Run Number:

S2-O-4CH-250918-115 & 22

Sample Name:


Manufacture & Expiration Date:

2025-Sep-18 & 2026-Mar-17

Sample ID: 8-20260319

Alignment Marker:

UserDefine (20 bp & 5K bp)

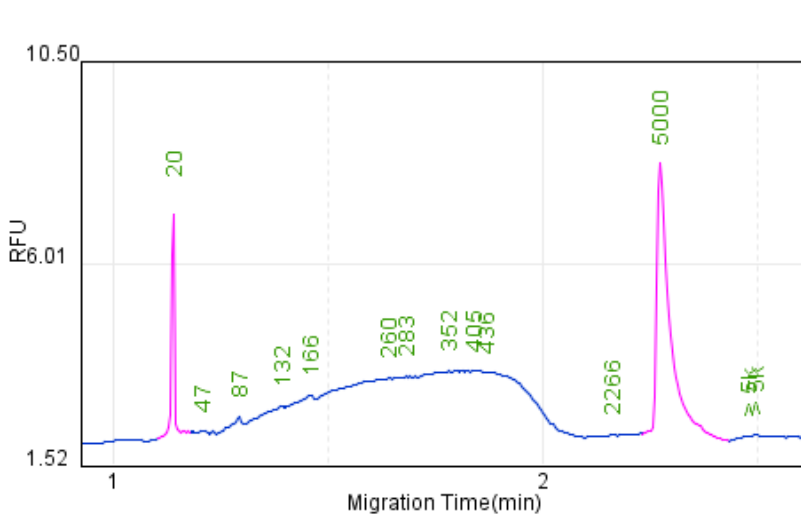

No	bp	ng/μl
1	20	N/A
2	37	0.01
3	47	0.04
4	59	0.02
5	87	0.15
6	132	0.38
7	166	0.27
8	260	1.42
9	271	0.19
10	283	0.22
11	295	0.09
12	337	0.59
13	352	0.15
14	367	0.12
15	375	0.11
16	388	0.12
17	405	0.30
18	436	0.99
19	1,795	<0.01
20	1,922	<0.01
21	2,266	<0.01
22	2,772	0.01
23	3,680	0.01
24	5,000	N/A
25	> 5k	N/A
26	> 5k	N/A
27	> 5k	N/A
28	> 5k	N/A
29	> 5k	N/A
30	> 5k	N/A
31	> 5k	N/A